

1/5

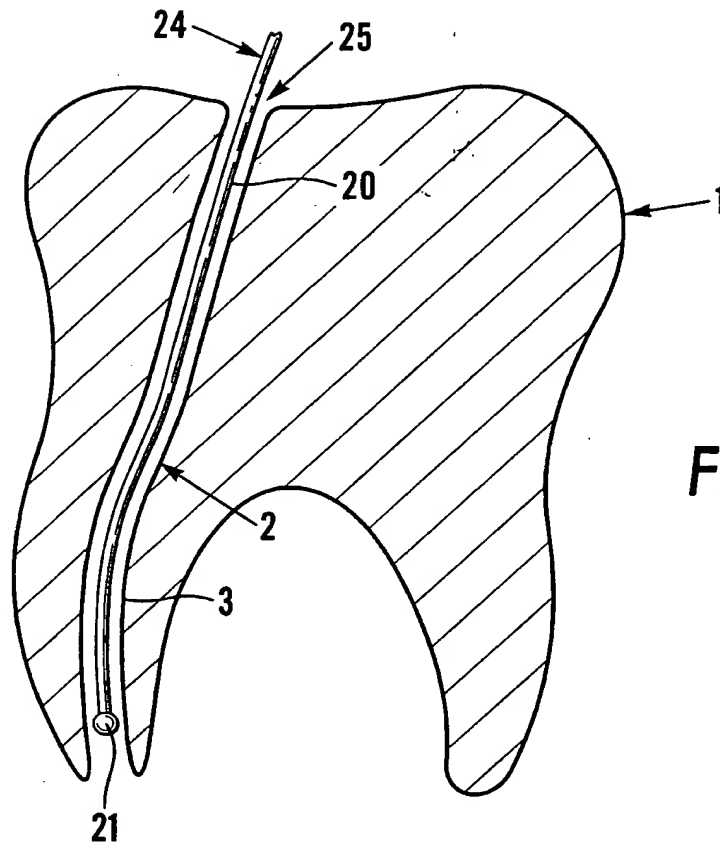


Fig. 1

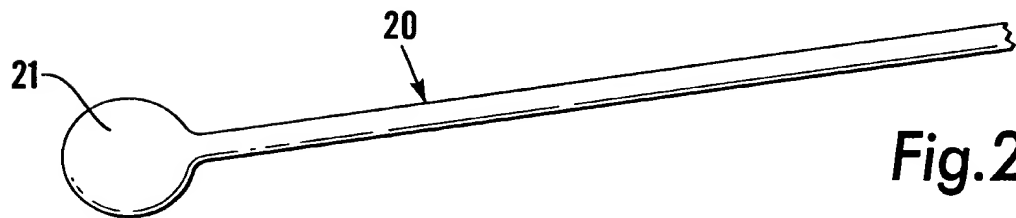


Fig. 2

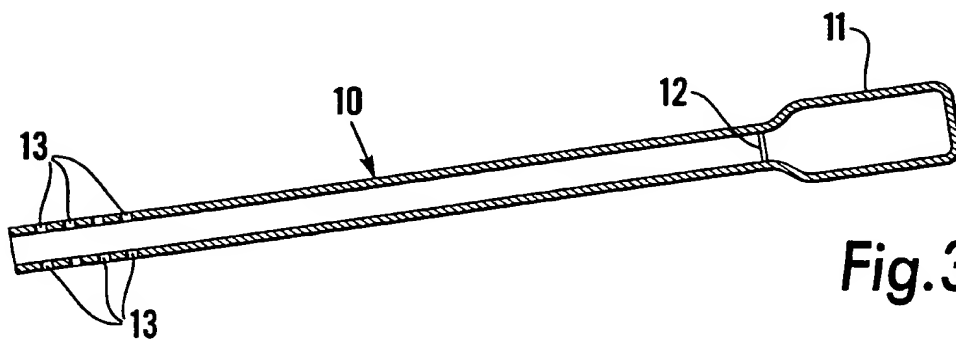


Fig. 3

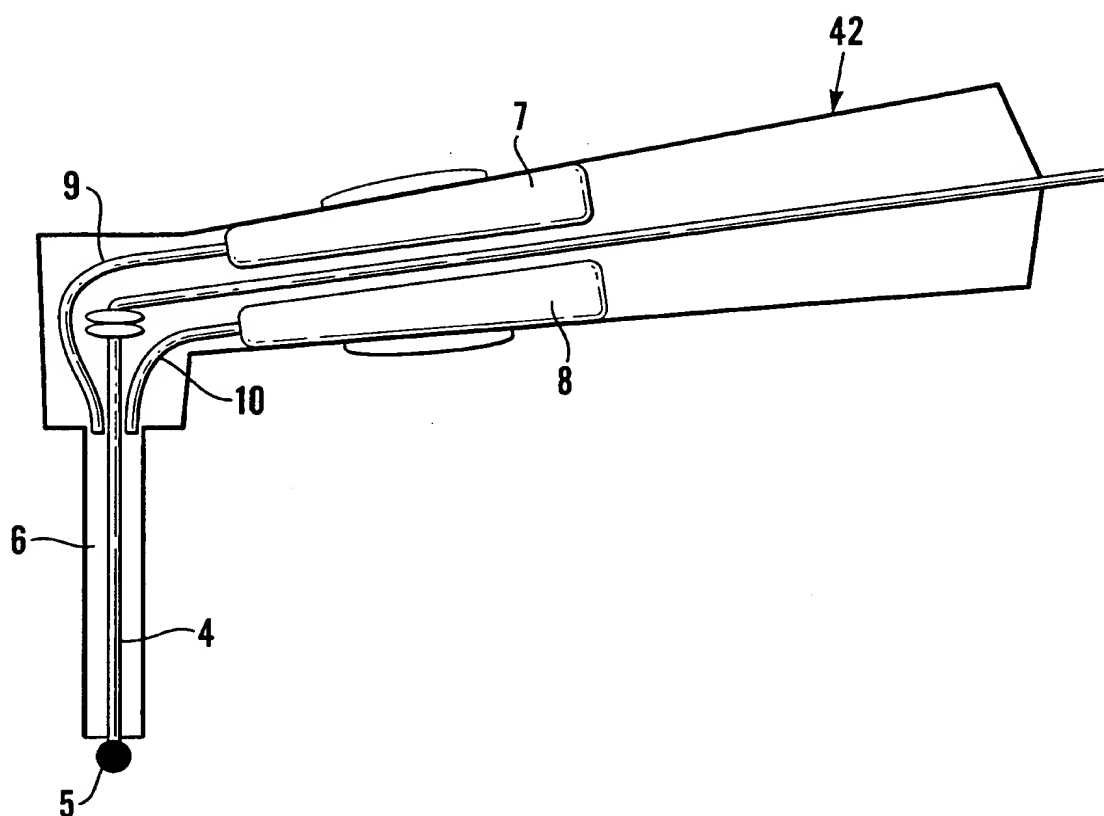


Fig.2a



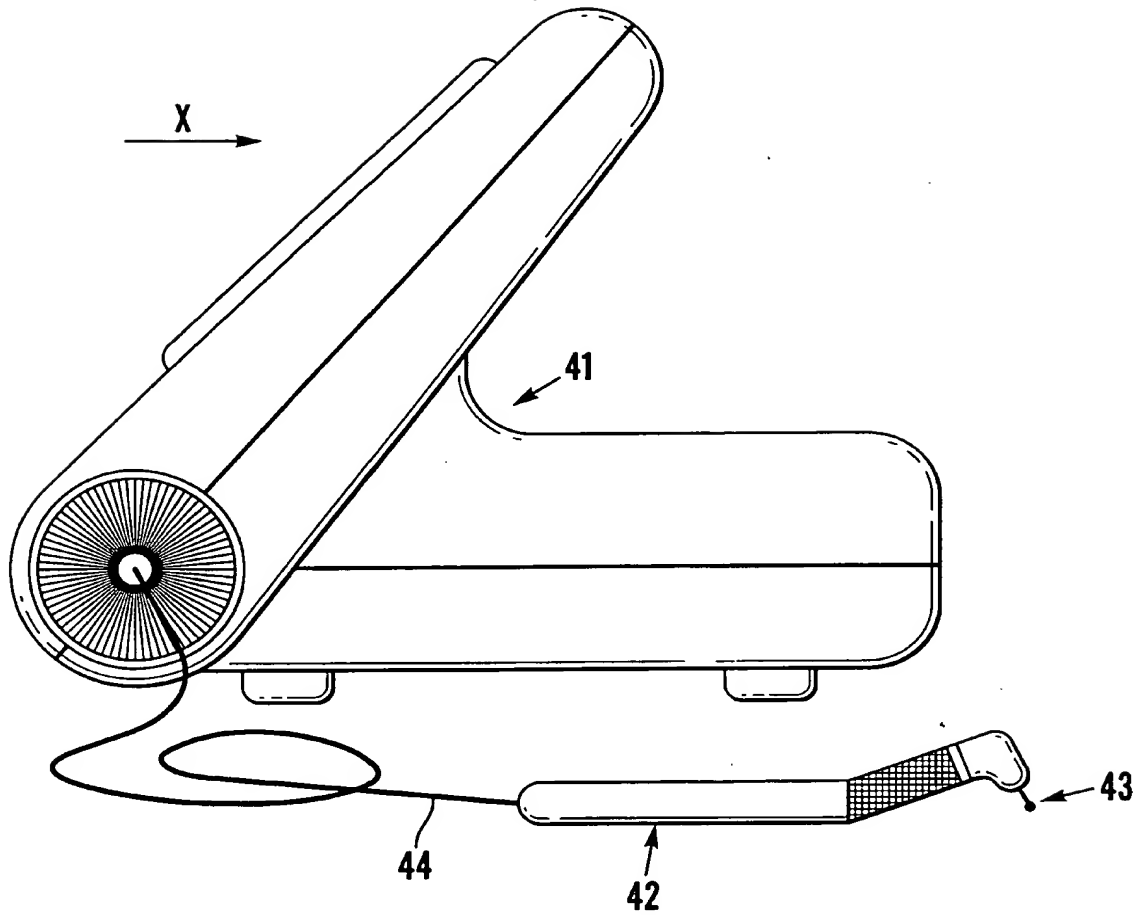


Fig.4



*Fig.5*

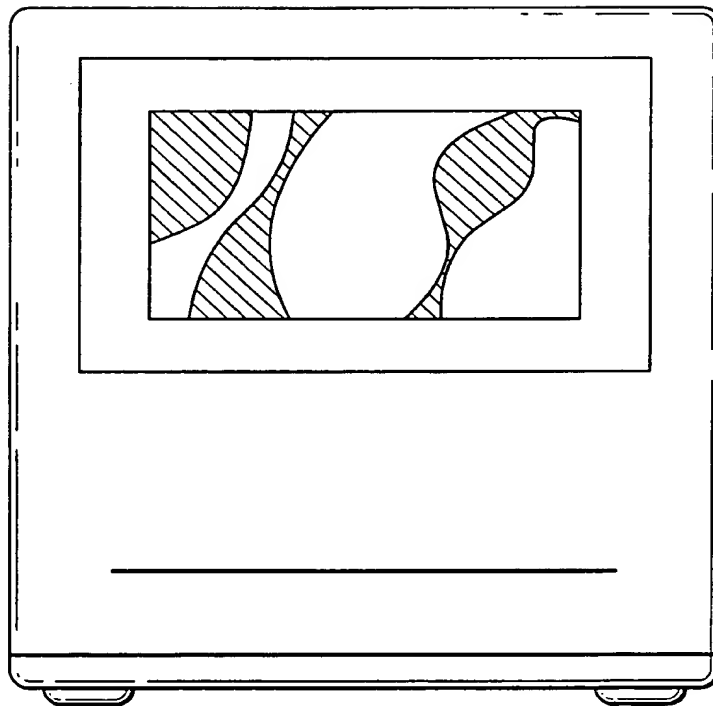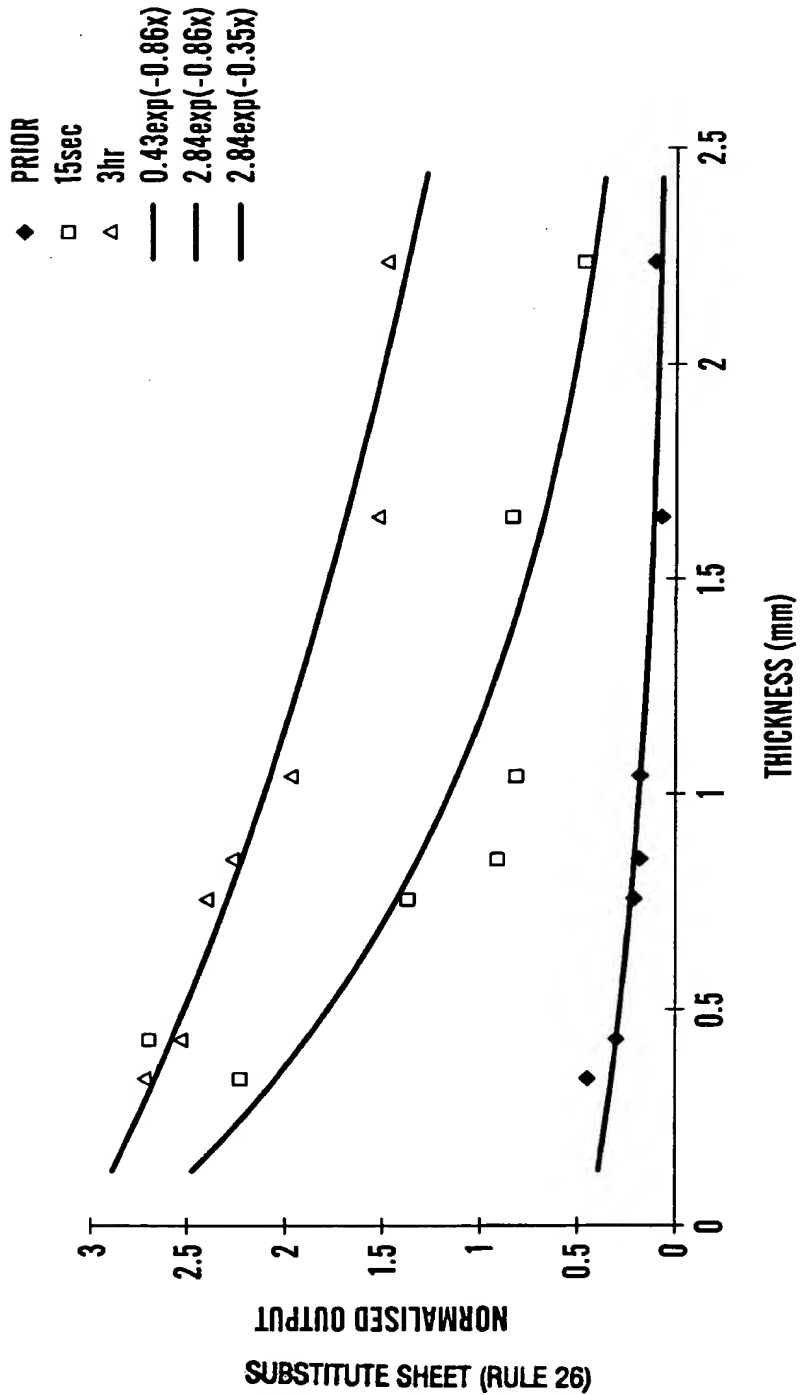

LIGHT DETECTED VS. THICKNESS FOR HORIZONTAL DISCS OF DENTINE FOR VARIOUS PROCESSING TIMES

Fig.6